

JH-338-4





Product feature

- 1.Rechargeable
-Micro USB charging dock , can work 16 hours after 8hours charging
- 2.Stable and Reliable
-Classic Design with Good quality
- 3.Easy Operation
-Simple slider key operation for volume
-Classic rocker-key operation to turn on and off, more adapt to the operation habits of the elderly
- 4.Moving coil loudspeaker in the ear, great gain;
- 5.Rotated tube, fit for either ear;


Technical Data	IEC 60118-7:2005 Test Data (2cc-coupler)	ANSI S3.22-2003 Test Data (2cc-coupler)
Operating Voltage	DC 1.0V~1.5V	DC 1.0V~1.5V
Acoustic Gain (50 dB SPL)		
HFA	38.7dB	38.6dB
1600Hz	42dB	42.5dB
Peak Value	45.7dB	/
Max. output		
HFA	121.4dB	121.4dB
1600Hz	121dB	122dB
Peak Value	126.8dB	126.8dB
Reference Test Gain	38.8dB	38.8dB
Induction Coil Sensitivity	/	/
Frequency Range	368Hz~3962Hz	370Hz~3960Hz
Total Harmonic Distortion(500/800/1600Hz)	3.1%/2.1%/0.3%	3.4%/1.8%/0.3%
Equivalent Input Noise	28.5dB	27.8dB
Battery Current	1mA	1mA
Battery Type	NI-MH battery	NI-MH battery
Working Time	16h	16h

FITTING RANGE

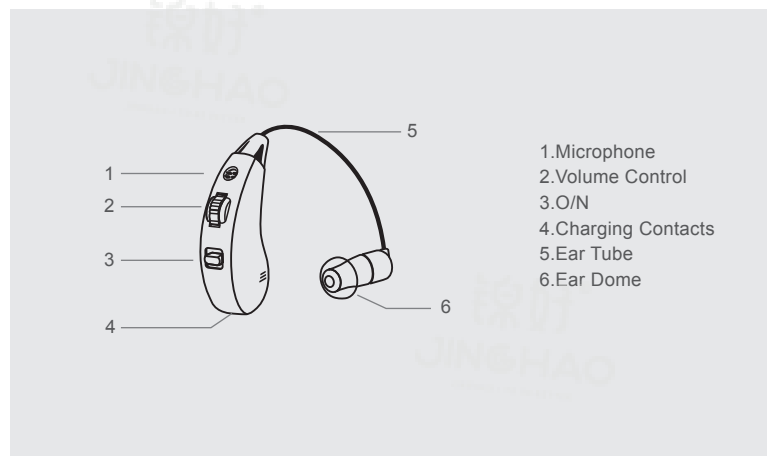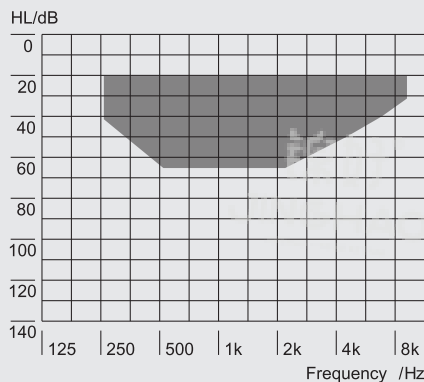

JH-338-4

Accessories




Ear Dome(L)




Ear Dome(M)



Ear Dome(S)




Micro USB charging dock




Cleaning tools

All Curves are measured with fonix 8000 hearing aid test system, 2ccm-coupler ,IEC 60118-7.All sound pressure levels are referred to 20μPa (OSPL90 Output/FOG50 Gain/Reference Test Gain(RTG))


OSPL₉₀ Output

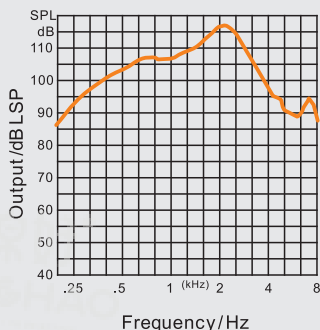

FOG50 Gain

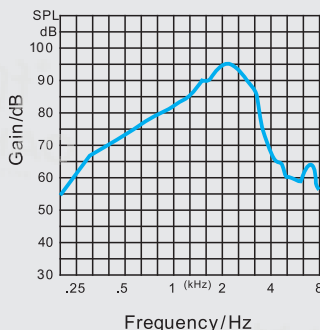

Reference Test Gain (RTG)

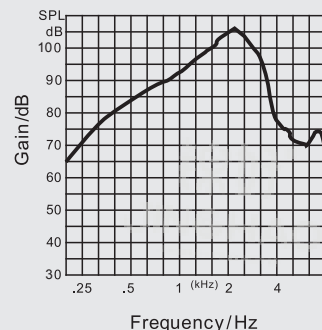

WARNING! Choking hazard posed by small parts. Infants, small children and persons of mental incapacity must not wear the hearing instrument without appropriate supervision.